Pressotherapy System

SE-BC05 User manual

Http://www.SPAelf.com

Introduction and function:

This machine adopts microcomputer control, easy to operate, not only for the beauty salon for a special diet and detox, but also suitable for dizziness, headache, neurasthenia, high blood cholesterol, waist, leg pain due to the nervous system, blood system, digestive system and secretion disorders, as well as variety of causes constipation due to mental stress and full psychosis and menopause comprehensive, achieving prevention and health functions, which is a multi-purpose functional excellence machine , to relieve the pressure of hunman, a good healthsecurity, family, and a must-new darling. Carefully before using this product, read the instruction manual and the correct use of the operation.

(1) It plays a role for the internal circulatory system in the human body : it is mainly directed against the body's internal circulation system. Internal circulatory system including: blood circulation, lymphatic circulatory system and tissue fluid, etc. Spacesuit through tightly tied to the customer abdominal, thigh, calf at the air bag, 16 seconds of each cycle for doing cycle-inflated, deflated, prompted acceleration cycle of the internal circulatory system in the human body. The body will produce the following effects:

1. Lymph drainage blood circulation system: promote blood circulation, especially can promote capillary blood circulation, accelerate blood circulation system, lymphatic system, tissue fluid circulation and exchange, better able to eliminate waste and toxin in the blood, consume and eliminate blood fat cells that adherent to the vascular wall, have very good prevention and health care function for atherosclerosis and high blood fat. Due to the blood circulation stagnant and lack of oxygen from blood, cause dizziness, headache, limbs cold, varicose veins, etc symptom, have better ease effect on them, can make whole blood circulation system fully purification.

2. Lymphatic system: lymphatic system has manufactured lymphocytes filter foreign objects swallowed toxins and produce antibodies roles, and hematopoietic and immune function. It is one of the human epidemic prevention system. Regular under pressure to accelerate the lymph reflux, stimulate the lymphatic vessels. Generating a large number of lymphocytes, accelerate the flow of the lymph and blood, tissue fluid and exchange, the nutrients will be back to the blood in the tissue fluid phagocytic toxin. Excess nutrients in the blood and tissue fluid, and the dissociated fatty be rapidly consumed and decomposition.

3. Tissue fluid: States to strengthen the tissue fluid circulation, better able to the blood supply of nutrients, concentrated a lot of waste, toxins, free state fat for lymphocytes swallowed. Its waste, toxins and excess water, after will be excreted by the metabolic system.Therefore, for against the edematous tissue cellular obese have significantly improved.

(2)Enhanced role in human metabolism: the whole within the circulatory system of the human body activity and body fluids purification, obviously increase metabolism. Meanwhile, in the rhythm of the pressure and vibration massage effect, the size of peristalsis accelerated digestive also become very active, so that excess nutrients and free state of fat, the body of excess moisture, metabolic waste, etc., through the urine smooth excreted. Therefore, a variety of causes constipation and to treat internal obese (such as spilled beer belly).

(3)The role of subcutaneous adipose tissue and muscle tissue: the machine application of traditional Chinese medicine principle, massage tied up parts of the rhythm, so that the muscle tissue to generate static aerobic consumption, break down fat and muscle were mixed and. Its unique high frequency vibrator, as needed affixed to the air bag on the abdomen, thighs, calves, by five thousand revolutions per minute standard vibration frequency, fatigue, muscle relaxation. Inflated state when the application site, which produces a powerful resonance force directly to the subcutaneous fat deep subcutaneous fat quickly loose, decomposition, also have separate handheld oscillator with prominent colloidal massage neck, soles of the feet and other parts, the elimination of body various parts of the aches, fatigue good. Conditioning of the body's internal and external treatment by the aircraft, so slimming, detoxification, health integration, both inside and outside primary care after people filled with energy, no weariness, is the best choice for healthy weight loss.

Panel graph:

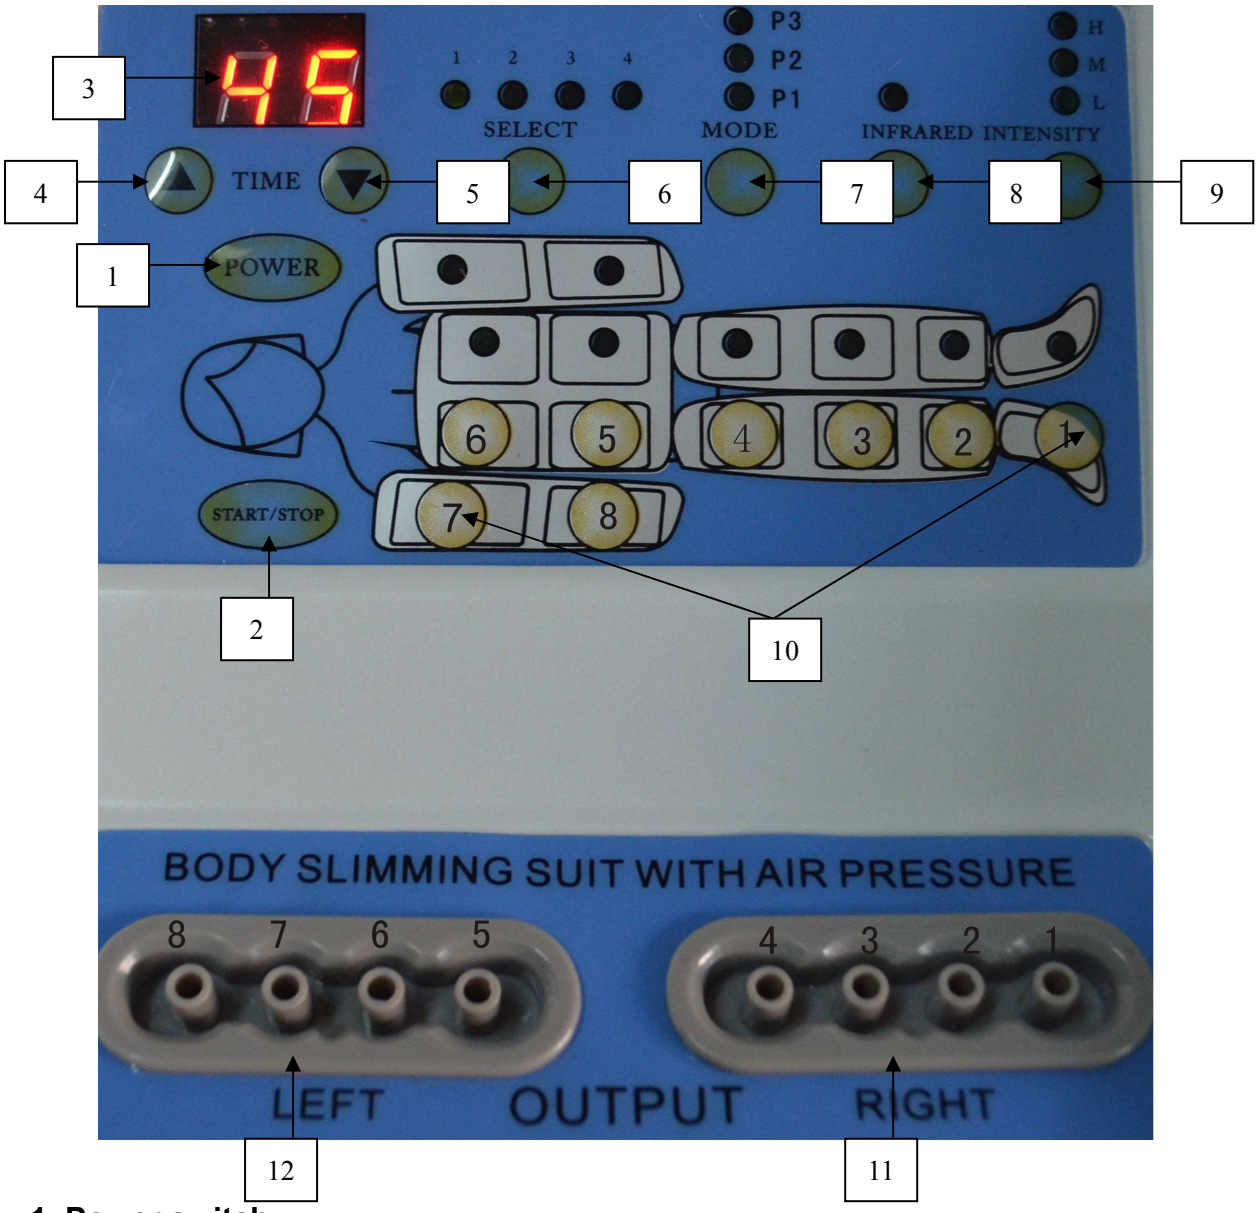

1. Power switch
2. Start/Stop button
3. Timer display
4. Time increasing
5. Time reducing
6. Time adjustment of air inflation
7. Modes of air inflation
8. Hot switch button
9. Hot level adjustment（L:large M:medium S: small）
10. 8connectors of are inflation output
11. Air inflation connectors (from right to left, from 1 to 4, in turn order)
12. Air inflation connectors (from right to left, from 5 to 8, in turn order)

Operation:

1. Connect various accessories to rear of the instrument accessories interface, plug in the power, strat the instrument, the instrument enters to the standby state, press the the POWER power switch on the instrument panel, the instrument gets into the working state, the default time is 45 minutes(time can be adjusted freely).
2. Working hours can be easily adjusted. P3 mode for 1-15 minutes; P2 mode for 15-30 minutes; P1 mode for 20-45 minutes, choose P(...) modes is the work mode for more than 45 minutes.
Note: The work state that interface, the lights flash on behalf of the inflated and deflated the lamp.
3. P1,P2,P3 are the **Air inflation** modes: P1, P2, is the default **Air inflation** mode, can not select the **Air inflation output** interface, P3 is any selectable mode, having a tapping function.
4. Press SELECT (1,2,3,4) to **Air inflation** time selection key: 1 is 10 seconds; 2 is 14 seconds; 3 is 17 seconds; 4 is 20 seconds. This tapping mode, the specific time such as the reference to this feature is only under P3 mode, each inflatable time three tapping mode, see reference table in detail.
5. The 8 **Air inflation** output on panel, the eight keys also represents the corresponding output pneumatic interface. Note only the P3 mode can be used to select as you need to work by any output Inflatable interface.
6. INFRARED is hot switch button, we must firstly open the switch, can adjust the INTENSITY heating level button.

Reference:

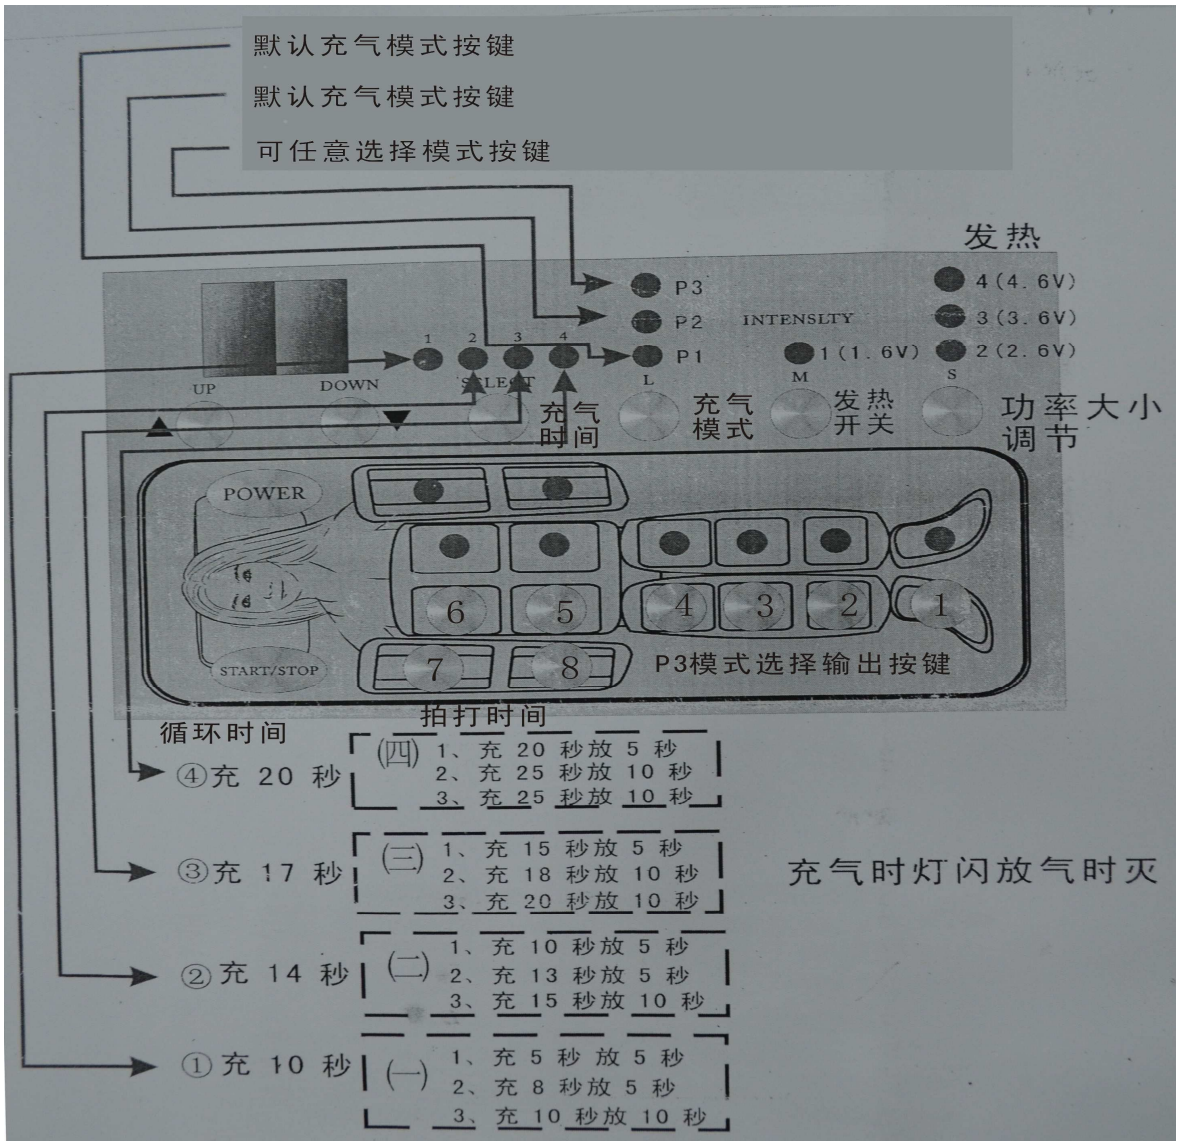

Instructions for use: Open the POWER button, select your model and inflation time.

For example: P1 mode is inflatable time,1 with 8 two inflatable interfaces at the same time work 10 seconds after, to 2 with 7, followed by 3 with 6,4 with 5 complete cycles work. P1, P2 mode work together is opposite of P1, first 4 with 5 and then to 3 with 6, followed by 2 with 7, the last 1 with 8 . Click to the work cycle of the output order, when using the two modes have two different massage effect.

P3 mode you can choose the output inflation port to work as you need, to choose a good inflatable time, and it has three tapping modes with three different effects each inflatable time, details such as the reference:

For example: You choose 1,2,5 three output inflatable connectors, inflatable time, then start working from 10 seconds of “1” to “2” to “5” is completed. All of deflation

for the first round of tapping mode, inflate 5 seconds, deflate 5 seconds. In the second round, inflate 8 seconds, deflate 5 seconds. In the third round, inflate 10 seconds, deflate 10 seconds to complete in order to enter the three output ports inflatable tapping mode to complete three flapping cycle work, turn the mode, choose output inflatable hole, to start tp work accordance with the reference.

Interface graphical

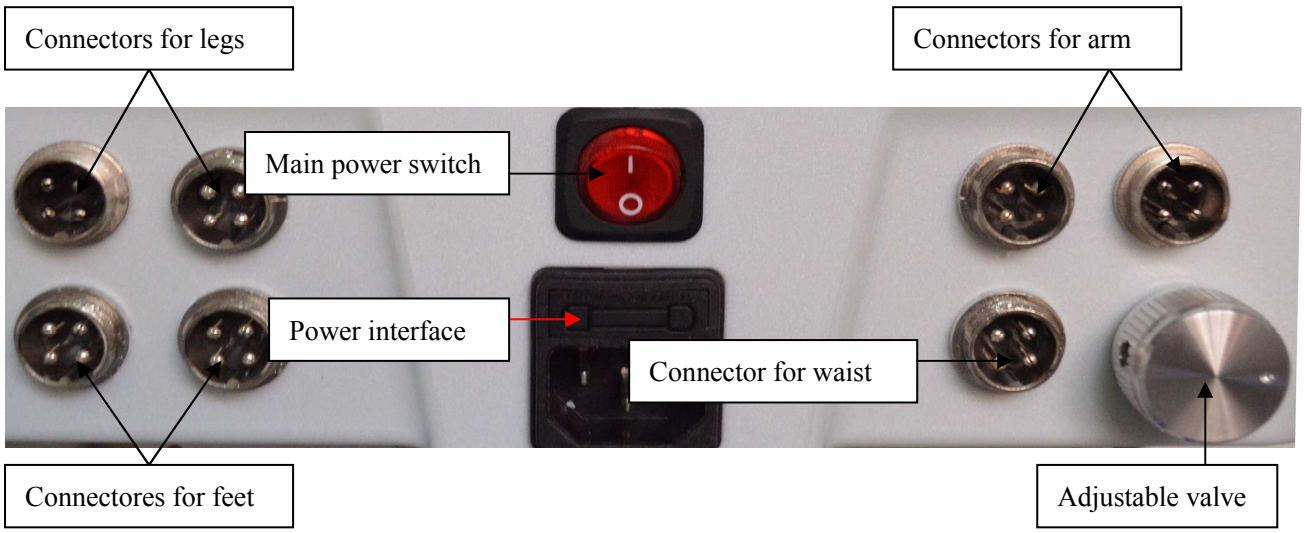

Working principle

The lymphatic detoxification slimming machine is known as the human body "scavenger", mainly within the circulatory system of the human body. The inner recycle including: the blood circulatory system, the lymphatic circulatory system and tissue fluid, etc. The air inflation by the air bag tie customers' abdomen, arms, legs lymphatic at inflated circulation to a certain period of time and deflated, prompting within the circulatory system to speed up the cycle in the human body, in order to achieve detoxification slimming, endocrine regulation.

Function characteristics

1, Body sculpting, weight loss, decomposition and eliminate stubborn fat.
2. Pneumatic detoxification, eliminate fatigue, relieve stress and muscle pain.
3, Promote blood circulation, improve metabolism.
4, Improve the systemic lymphatic system and the organization of loose skin.

Air pressure lymphatic drainage lossing weight is to promote the normal flow of lymph through the instrument, and waste from the body, which is different from the last patch vibration of the instrument it is with the airbag pressure and surface fat movement. Beauticians use basic techniques, plus the instrument the help of specialized lymphatic drainage, circulation, massage, rotation, traction accelerate lymphatic circulation and excretion, so that kept clear to facilitate the removal of waste. Gas wave-style soft natural air massage will not cause any harm and bad feelings at the same time the the airbags one-sided pressure equivalent to 50kg weight, acting on the abdomen 30 minutes is equivalent to 150 sit-ups exercise.

Physical therapy effect

1. Improve the shoulder, cervical and lumbar spine.
2. Enhanced cell potential film and to improve and slow organ aging (such as: kidney, gastrointestinal disorders)
3. Breast massage: treatment of lobular hyperplasia.
4. Eliminate constipation.
5, Slim (to improve local obesity).

Precautions

During the operation, in addition to the available intensity adjustment key to adjust the level of the pressure, but also, depending on the parts of the body is exposed to pressure, appropriately adjusting the tightness of the parts of the air bag to adjust the size of the pressure. Against the abdomen care should be aimed at the abdomen, so that the abdomen airbagthe bag inflatable parts are the abdomen, and the air bag down as far as possible, snapping abdominal position, to prevent the air bag from direct compression of the heart, causing discomfort to the customer. Customers need a back massage care, inflatable parts are on the waist. The thigh airbags should be up close to the thigh, to stimulate the abdominal muscles sulcus lymph.

Precautions

1, Customers must remove all metal objects before operating. Pressure energy regulation level and clothes size freely adjusted the size of the actual situation according to guests
2,Discomfort in body and pregnant women customers are not recommended to use this machine. Customer within one hour after meal, you can not use the machine for care
3, After using, should be in accordance with the program to turn off the power, unplug the the air ducts plug, remove air ducts, remove various parts of the airbag,

do not be too ruld unfolding and belongs accessories properly kept in accordance with the requirements. Disinfect and clean clothes and machine.

Technical parameters

Voltage: 110V/120V-220V/240V
Frequency: 50 Hz - 60Hz
Power: ≤300W
Safe voltage output：36V
Heat output：30℃-65℃
Material: ABS
GW/NW：
Packing size：

Part list

1、Host 1
2、Power line 1
7、Instruction 1

Product service and repair

1. This machine from the date of purchase (with a note) host a year warranty. Quality problems within one year have free repair, such as the problems after one year will receive maintenance costs. Parts' warranty for six months; in six months appear quality problem have free repair by free of charge; after six months charge parts maintenance costs. Other has been guarantee deadline, can

be responsible for maintenance, but charge spare parts and consumables cost fee. If need supplement or purchase, please contact our company.
2. Causes the following use of personal failure, does not provide free warranty service.
1) The unauthorized entry, modification caused the failure of the product;
2) Use accidentally blows, falls caused by the fault;
3) Lack of reasonable maintenance caused the failure;
4) Did not at the correct guidance of instructions caused by the fault.